



## White paper

## Standardizing terms for tribocorrosion-associated adverse local tissue reaction in total hip arthroplasty

Brian J. McGrory, MD, MS<sup>\*</sup>, Joshua J. Jacobs, MD, Young-Min Kwon, MD, PhD,  
Yale Fillingham, MD

Department of Orthopaedic Surgery, Tufts University School of Medicine, Boston, MA, USA

Department of Orthopaedic Surgery, Rush University Medical Center, Chicago, IL, USA

Department of Orthopaedic Surgery, Massachusetts General Hospital, Boston, MA, USA

## ARTICLE INFO

## Article history:

Received 4 January 2020

Received in revised form

19 January 2020

Accepted 21 January 2020

Available online 3 March 2020

## Keywords:

white paper

nomenclature

mechanically assisted crevice corrosion

(MACC)

adverse local tissue reaction (ALTR)

tribocorrosion

metal-on-polyethylene (MoP)

## ABSTRACT

Recognizing and adopting standardized terms for adverse local tissue reaction associated with tribocorrosion in total hip arthroplasty are essential for clear scientific discourse and clinical communication. Our goal was to develop terms that can be broadly applied to characterize the local tissue response to tribocorrosion debris, based on current evidence regarding the etiology of this failure mode and its consequences. The proposed standardized terms will improve the understanding and interpretation of analytical tests, advance diagnostic and treatment algorithms, and reduce confusion in research by maintaining consistent nomenclature.

© 2020 The Authors. Published by Elsevier Inc. on behalf of The American Association of Hip and Knee Surgeons. This is an open access article under the CC BY-NC-ND license (<http://creativecommons.org/licenses/by-nc-nd/4.0/>).

## Introduction

Tribocorrosion is defined as “an irreversible transformation of material in tribological contact caused by simultaneous physico-chemical and mechanical surface interactions” [1]. In other words, the discipline of tribocorrosion considers both the mechanical and electrochemical degradation of metallic materials in contact; the mechanical and electrochemical degradative processes for metal/metal interfaces are synergistic and must be considered together to achieve a complete understanding of the potential sequelae [2]. Tribocorrosion-related failure of contemporary metal-on-polyethylene (MoP) total hip arthroplasty (THA) has been recognized for decades but recently appears to have become more common, more recognized, or both (Fig. 1). In addition, revision specifically for this problem is also more frequent [3,4] and is recognized to have poor outcomes [5–8], with over one-fourth of patients experiencing serious complications including instability,

infection, and chronic pain. Different terms are used to describe this mode of tribocorrosion failure, including both terms for the breakdown at the metal/metal modular junction itself and also terms referring to an individual's biological reaction to this malfunction.


It is essential to standardize these terms to facilitate diagnosis, treatment, research, and interdisciplinary communication. To achieve this goal, particularly for purposes of uniform communication through peer-reviewed publication, *Arthroplasty Today* supports this project to identify terms that could be used consistently for tribocorrosion in MoP THA. When possible, the goal was to agree on uniform terms that could be applied to characterize (i) tribocorrosion failure mechanisms of the THA metal/metal modular junction and (ii) local biological reactions to tribocorrosion products produced from this failure.

## Problem statement

There is a lack of uniformity and specificity in the current terminology used to describe MoP THA failure due to in vivo tribocorrosion of metal/metal modular junctions and its biological consequences. The term “trunnionosis” is often used to describe a biological reaction, presumably inflammatory in nature, associated with the trunnion of the femoral component of a hip replacement.

<sup>\*</sup> Corresponding author. Department of Orthopaedic Surgery, Tufts University School of Medicine, Boston, MA, USA; Maine Medical Center Division of Joint Replacements, Portland, ME, USA. Tel.: +1 207 781 1551.

E-mail address: [mccgrb1@mmc.org](mailto:mccgrb1@mmc.org)

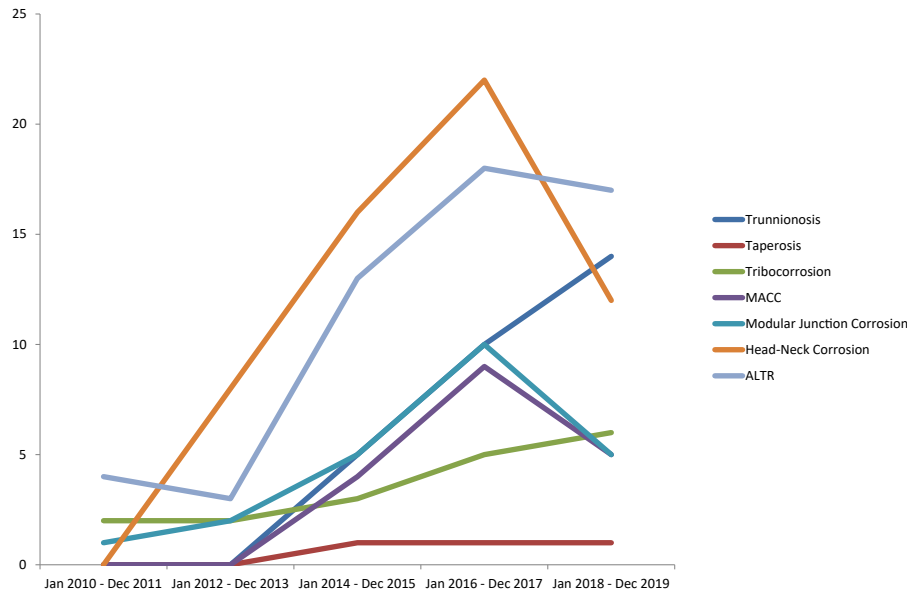

**Figure 1.** Graph demonstrating general increase in keywords used as search terms for tribocorrosion-related adverse local tissue reaction usage over the last decade in PubMed. PubMed is a free search engine maintained by the United States National Library of Medicine at the National Institutes of Health that accesses the MEDLINE database for life sciences and biomedical topics.

This oversimplification is not particularly useful, and the presumption of an inflammatory response may be misleading. Another term commonly used to describe a patient’s reaction to corrosive failure is “pseudotumor,” and this too is poorly defined and misleading. Metallosis refers to macroscopic black or gray stained tissues. Aseptic lymphocyte-dominated vasculitis-associated lesion (ALVAL) is not a clinical diagnosis; however, it represents histological appearance of tissues characterized by lymphocyte infiltration and perivascular cuffing [9]. Fluid alone on an MRI may be interpreted as an adverse local tissue reaction (ALTR) [10,11], and systems to grade these MRI changes show only moderate agreement among reviewers [12]. A group of other such terms and test parameters, often adopted from research of failed metal-on-metal (MoM) hip arthroplasties, adds to confusion in this field (Table 1).

The lack of standard vocabularies describing this failure mode further interferes with comprehension of patients, clinicians, researchers, and readers of medical literature. Uncertainty is observed in oral presentations as well as publications on this topic. The impact on communication may significantly impede the understanding and treatment of this method of joint replacement malfunction.

To be specific in the scope of this project, we will focus on standard, contemporary THAs. These definitions will also have applicability to other metallic implants where there are metal/metal interfaces that have the potential to release debris via tribocorrosion mechanisms, eg, modular stem extensions in total knee replacement.

**Table 1**  
Terms that may be confusing in current literature pertaining to adverse local tissue reaction (ALTR) in metal-on-polyethylene (MoP) total hip arthroplasty (THA).

Terms that are too general, misleading, or repetitive	Terms that are too specific and may be misleading if used out of context
<ul style="list-style-type: none"> <li>metallosis</li> <li>trunnionosis</li> <li>taperosis</li> <li>biocorrosion</li> <li>pseudotumor</li> <li>adverse reaction to metal debris (ARMED)</li> </ul>	<ul style="list-style-type: none"> <li>aseptic lymphocyte-dominated vasculitis-associated lesions (ALVAL)</li> <li>galvanic corrosion</li> </ul>


**Proposed solution**

We propose understanding in vivo tribocorrosion at modular metal/metal junctions of MoP THA in terms of 1) the underlying mechanism, mechanically assisted crevice corrosion (MACC) and 2) the patient’s biological response, ALTR. Of note, having the former, MACC, does not imply that ALTR must be present, but tribocorrosion-related ALTR cannot be present without MACC in contemporary MoP THAs.

*Mechanically assisted crevice corrosion*

Retrieval and clinical studies have shown that both mixed-alloy (Ti-6Al-4V stems and Co-Cr-Mo heads) and similar-alloy (Co-Cr-Mo stems and Co-Cr-Mo heads, and Ti-6Al-4V stems and Ti-6Al-4V heads) couples sometimes demonstrate in vivo corrosion [3,4,13] (Fig. 2). There is some controversy as to whether this is more common in mixed-alloy settings [13,14], which highlights the need for additional research to clarify this finding because there may be bias introduced by evaluating only retrieved implants (retrievals are primarily failed total hips, and corrosion may contribute to a failure, without being recognized [15,16]). Furthermore, retrieval laboratories estimating prevalence of corrosion based on visual inspection may have poor accuracy for lower grades (Goldberg 1-2) [17]. It is important to know that not all modular hip replacements corrode [3,14,18], and in one sample of symptomatic THA patients with a contemporary titanium alloy stem and cobalt alloy femoral head, 51.1% of patients with symptoms had serum Co less than 1 ppb, at an average of 60.1 months after index THA [3]. A further cohort from the same institution demonstrated 60%-75% of all patients from a single year studied had a serum Co < 1 ppb 10 years postoperatively [19]. In addition, Levine and colleagues showed that well-functioning hips, followed over a 10-year span, also had serum metal levels less than 1 ppb. They did note, however, that serum Co levels increased over time for the subset of patients with hybrid Co-Cr-Mo stems and Co-Cr-Mo heads [14].

The corrosion process is thought to be the result of mechanical-electrochemical interactions in the taper crevice. Metal implants all

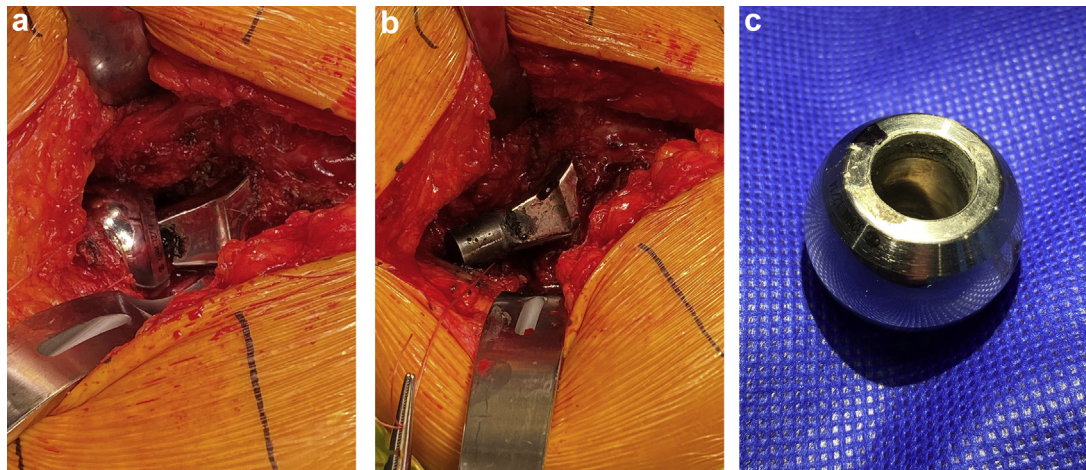

**Figure 2.** Mechanically assisted crevice corrosion (MACC) describes the underlying mechanism of significant tribocorrosion at the femoral trunnion-head bore junction, as seen in these clinical photographs: (a) dark material noted at base of junction of the head and trunnion in a failed metal-on-polyethylene (MoP) total hip arthroplasty (THA), (b) marked discoloration of trunnion after removal of femoral head, (c) marked discoloration of bore of femoral head with transfer of trunnion markings (so-called “stamping”).

have passivation of their surface, a continuous, protective, oxide layer that protects against further oxidation and corrosion. In cases of MACC, the passivating oxide film disruption caused by fretting and the constrained crevice environment of the modular junction combine to cause changes in the fluid chemistry inside the taper (including decreases in pH and increases in chloride concentrations) [20]. Furthermore, the potential of the implant becomes significantly more negative, and this, in turn, causes the passive oxide layer which reforms to be thinner than the original film [21]. Loading of THAs during activities of daily living causes stress and possibly micromotion at the taper interface, leading to recurring disruption of the passive layer on the implant surface. The exposed metal substrate then spontaneously reoxidizes *in vivo*. This causes additional oxygen depletion in the fissure, thereby accelerating the process of crevice corrosion, including the release of metal ions and solid particles [22,23].

Fretting involves more severe mechanical damage to the metal surface. Deep-surface asperities form beyond the passive layer and consequently provide further sequestered electrochemical environments for pitting corrosion. Once fretting starts, the corrosion processes may continue in the absence of loading [17]. Some retrieved tapers show evidence of etching and grain egression (a mechanism of fatigue-crack initiation) at these interfaces, suggesting macroscopic movement [24]. Furthermore, corrosion at the interface may lead to instability and macromotion, making them further susceptible to abrasive wear [17,24,25], although this may be prosthesis specific [16].

This process is referred to as MACC and we propose that this term be used to describe the underlying mechanism of significant tribocorrosion at the femoral trunnion-head bore junction, the femoral neck-stem junction in modular neck devices, the metal acetabular liner-shell junction, and other metal/metal modular connections (Table 2). The discoloration and debris are likely a combination of tribocorrosion mechanisms and may or may not lead to discoloration of the surrounding tissues or joint fluid. Ideally, retrieval analysis with a coordinate measuring machine to assess material loss due to corrosion could confirm with certainty the diagnosis of MACC [26].

The products of tribocorrosion generated from MACC vary in size from <1 to 500 micrometers [27]. Most particulate debris is <5 micrometers in size and plate shaped, irrespective of the material combination used [27,28]. The most abundant particles produced are chromium orthophosphate (CrPO<sub>4</sub>) and mixed oxides; but

chlorides of chromium, molybdenum, and titanium (Ti) are also common [27]. The biological response to these corrosion products is similar to that produced by MoM bearing surface debris [4] but there is evidence suggesting that tribocorrosion products may be more biologically active and highly necrotizing [29], possibly as a result of higher concentrations of ionized metal and chemokines [29,30].


MACC is therefore associated with elevated intra-articular Co levels (greater than 100 ppb [29,31,32]) and through diffusion, phagocytosis, and other means—serum, whole blood, cerebrospinal fluid, urine, and solid organ levels are also elevated. Peripheral metal levels in MACC are significantly lower than in the tissues directly around the implant because of dilutional effects, renal excretion, and possibly necrosis of joint tissues impeding diffusion

**Table 2**

Proposed terminology and criteria for terms referring to triobocorrosion-related findings in contemporary total hip replacement (THA) including mechanically assisted crevice corrosion (MACC) and adverse local tissue reaction (ALTR).

Terminology	Criteria
MACC	Retrieved femoral head with evidence of tribocorrosion damage (Goldberg grade 2 or higher)
ALTR (one or more of these)	<ol style="list-style-type: none"> <li>1. Osteolysis on radiographs and no evidence of infection or wear in patients with cross-linked polyethylene when there is concomitant evidence of MACC either by direct observation intraoperatively or by findings of elevated blood cobalt levels.</li> <li>2. Cross-sectional imaging (MARS-MRI; ultrasound or CT scan when MRI is contraindicated or MARS not available) demonstrating abnormal tissue reactions involving surrounding muscle and/or bone and cystic lesion(s) surrounding the hip when there is concomitant evidence of MACC either by direct observation intraoperatively or by findings of elevated blood cobalt levels.</li> <li>3. Intraoperative finding of osteolysis, devitalized tissue, bone necrosis, muscle necrosis, tendon detachment, capsule dehiscence, capsular thickening, cystic lesion(s), excessive fluid collection(s), and soft tissue masses when there is concomitant evidence of MACC by direct observation intraoperatively. These gross findings may be present with or without metal staining of the tissues.</li> <li>4. Histopathology from biopsy or from a revision with dense infiltrates of perivascular lymphocytes (ALVAL) and/or areas of tissue necrosis when there is concomitant evidence of MACC either by direct observation intraoperatively or by findings of elevated blood cobalt levels.</li> </ol>



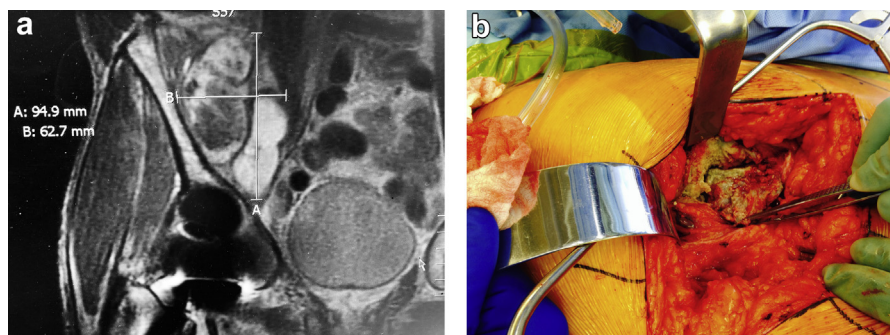

**Figure 3.** A significant local biological reaction noted in a high proportion of cases of MACC is referred to as an adverse local tissue reaction (ALTR), as is exemplified by (a) a periarthritic mass noted on metal artifact reduction sequence (MARS) magnetic resonance imaging (MRI) in this patient with elevated serum cobalt (Co) and chromium (Cr) levels and new-onset hip symptoms and (b) a clinical photograph of a different patient with a MoP THA, progressive hip weakness, and a pathological local biological reaction attributed to MACC.

[31]. Of note, serum Co levels are disproportionately greater than Cr in MACC (4–5:1) in both intra-articular and systemic measurements. Cr is less soluble than Co and can precipitate as CrPO<sub>4</sub> (chromium orthophosphate) or other species. Therefore, the concentration of Cr is less in the bloodstream and is more persistent in the local tissues.

#### *Adverse local tissue reaction*

ALTRs are pathological local biological tissue reactions that occur in direct approximation to a MoP hip joint that has significant tribocorrosion (Fig. 3). Reactions may include osteolysis, bone necrosis, muscle necrosis, tendon necrosis with or without detachment, capsular necrosis with or without dehiscence, capsular thickening, cystic lesion(s), excessive fluid collection(s), ALVAL, and soft tissue masses [10,11,33–37]. Many of these features are seen in variable amounts in cases of ALTR and it is not clear why some lesions show a predominance of one feature over the others. Although these reactions originate locally, they may extend into the surrounding tissues, local lymph system, muscular planes, and may even cause obstructive vascular or neurological compromise [8,38,39]. The cause of ALTR is most likely multifactorial and both local Co toxicity [29,31,32] and a delayed-type hypersensitivity-like immune response (aseptic lymphocyte-dominated vasculitis-associated lesion or ALVAL) may be operative [35]. Furthermore, the adaptive immune response or hypersensitivity may play an important role in the pathogenesis of these ALTRs in a subset of patients, but current diagnostic tools for metal hypersensitivity have yet to be clinically validated [40]. Patients with an ALTR may or may not be symptomatic [19].

A significant local biological reaction noted in a high proportion of cases of MACC (49% on initial presentation in one study [3]) is best referred to as an ALTR and we propose that this term is used to describe all cases of pathological local biological reaction attributed to MACC. A serum Co of >1 ppb has been shown to be associated with both tribocorrosion and associated ALTR [34,37]. It is acknowledged that MRI abnormalities may not be significant in patients without MACC [10], but such findings are likely to be important in patients with MACC [3,19].

#### **Future direction and long-term focus**

We hope that this proposed general terminology be used in clinical practice, research publications, and other communications when describing tribocorrosion damage and its local biological sequelae associated with MoP THA with metal/metal modular junctions. Furthermore, we recommend that world registries,

including the American Joint Replacement Registry, refine diagnostic codes (both primary and secondary) adopting these criteria for MACC and ALTR relating to THA failures and revisions. Such codes could also be added as a set of supplementary codes for the 10th revision of the International Statistical Classification of Diseases and Related Health Problems.

#### **Recommendations**

We propose that clinicians, researchers, and authors describe the mechanism of in vivo tribocorrosion at metal/metal modular junctions of THA using the term MACC, and patient's local biological response using the term ALTR. We want to reiterate that all hip implants do not demonstrate MACC and that an ALTR appears to occur at presentation in only some cases of MACC.

#### **Conflict of interest**

Brian J. McGrory, MD, MS, reports royalties from Innomed, Inc., Smith & Nephew, Inc.; Speakers bureau/paid presentations and paid consultant for Smith & Nephew, Inc. Joshua J. Jacobs, MD, Paid consultant for Consultant, Zimmer Biomet, Stock for Hyalex; Research support Medtronic, Nuvasive; Royalties, financial or material support Secretary of the Board of Trustees, Journal of Bone and Joint Surgery; Medical/Orthopaedic publications editorial/governing board Secretary of the Board of Trustees, Journal of Bone and Joint Surgery; Board member/committee appointments for a society President, The Hip Society; Vice President, American Board of Orthopaedic Surgery; Treasurer, Orthopaedic Research and Education Foundation. Young-Min Kwon, MD, PhD, Institutional Research support as a Principal Investigator from the following companies – Smith & Nephew, Zimmer Biomet, Stryker, Corentec; Yale Fillingham, MD, Paid consultant for Johnson & Johnson, Medacta; Stock Muvr Labs, Inc.; Board member/committee appointments for a society AAOS, EBVQ Committee Member and AAHKS, YAG Committee Member.

For full disclosure statements refer to <https://doi.org/10.1016/j.artd.2020.01.008>

#### **References**

- [1] Landolt DMS, Stemp M. Electrochemical methods in tribocorrosion: a critical appraisal. *Electrochim Acta* 2001;46(24–25):3913.
- [2] Matthew M, Jacobs J, Wimmer M. Wear-corrosion synergism in a CoCrMo hip bearing alloy is influenced by proteins. *Clin Orthop Relat Res* 2012;470:3109.

- [3] Hussey D, McGrory BJ. Ten-year cross-sectional study of mechanically assisted crevice corrosion in 1352 consecutive patients with metal-on-polyethylene total hip arthroplasty. *J Arthroplasty* 2017;32:2546.
- [4] Cooper HJ, Della Valle CJ, Berger RA, et al. Corrosion at the head-neck taper as a cause for adverse local tissue reactions after total hip arthroplasty. *J Bone Joint Surg Am* 2012;94-A(18):1655.
- [5] McGrory BJ, Jorgensen A. High early major complication rate after revision for mechanically associated crevice corrosion in metal-on-polyethylene total hip arthroplasty. *J Arthroplasty* 2017;32:3704.
- [6] Kwon YM, Rossi D, MacAuliffe J, Peng Y, Arauz P. Risk factors associated with early complications of revision surgery for head-neck taper corrosion in metal-on-polyethylene total hip arthroplasty. *J Arthroplasty* 2018;33:3231.
- [7] Waterson HB, Whitehouse MR, Greidanus NV, Garbuz DS, Masri BA, Duncan CP. Revision for adverse local tissue reaction following metal-on-polyethylene total hip arthroplasty is associated with a high risk of early major complications. *Bone Joint J* 2018;100-B:720.
- [8] Persson A, Eisler T, Boden H, Krupic F, Skoldenberg O, Muren O. Revision for symptomatic pseudotumor after primary metal-on-polyethylene total hip arthroplasty with a standard femoral stem. *J Bone Joint Surg Am* 2018;100(11):942.
- [9] Wilert H-G, Buchhorn G, Fayyazi A, et al. Metal-on-metal bearings and hypersensitivity in patients with artificial hip joints. *J Bone Joint Surg Am* 2005;87:28.
- [10] Fehring TK, Fehring KA, Odum S. Metal Artifact Reduction Sequence MRI abnormalities occur in metal-on-polyethylene hips. *Clin Orthop Relat Res* 2015;473(2):574.
- [11] Hjorth MH, Mechlenburg I, Soballe K, Roemer L, Jakobsen SS, Stilling M. Higher prevalence of mixed or solid pseudotumors in metal-on-polyethylene total hip arthroplasty compared with metal-on-metal total hip arthroplasty and resurfacing hip arthroplasty. *J Arthroplasty* 2018;33:2279.
- [12] Smeeks C, Schouten BJM, Nix M, et al. Pseudotumor in metal-on-metal hip arthroplasty: a comparison study of three grading systems with MRI. *Skeletal Radiol* 2018;47(8):1099.
- [13] Collier JP, Mayor MB, Williams JM, Surprenant VA, Surprenant HP, Currier BH. The tradeoffs associated with modular hip prostheses. *Clin Orthop Relat Res* 1995;311:91.
- [14] Levine BR, Hsu AR, Skipor AK, et al. Ten-year outcome of serum metal ion levels after primary total hip arthroplasty. *J Bone Joint Surg Am* 2013;95(6):512.
- [15] Lash N, Whitehouse MR, Greidanus NV, Garbuz DS, Masri BA, Duncan CP. Delayed dislocation following metal-on-polyethylene hip replacement due to “silent” trunnion corrosion. *Bone Joint J* 2016;98B(2):187.
- [16] Higgs GB, MacDonald DW, Lowell J, et al. Technical note: is corrosion a threat to the strength of the taper connection in femoral components of total hip replacements? *Corrosion* 2017;73(12):1538.
- [17] Goldberg JR, Gilbert JL. In vitro corrosion testing of modular hip tapers. *J Biomed Mater Res B Appl Biomater* 2003;64:78.
- [18] Lange J, Wach A, Koch CN, et al. Do well-functioning THAs retrieved at autopsy exhibit evidence of fretting and corrosion. *Clin Orthop Relat Res* 2018;476:2017.
- [19] McGrory BJ. High incidence of mechanically assisted crevice corrosion at 10 years in non-cemented, non-recalled, contemporary total hip replacement. Orlando, FL: AAOS; 2020.
- [20] Griess JC. Crevice corrosion of titanium in aqueous salt solutions. *Corrosion* 1968;24(4):96.
- [21] Gilbert JL, Jacobs JJ. The mechanical and electrochemical processes associated with taper fretting crevice corrosion: a review. In: Marlowe DE, Parr JE, Mayor MB, editors. *Modularity of orthopaedic implants*. West Conshohocken, PA: ASTM International; 1997. p. 45–59.
- [22] Gilbert JL, Buckley CA, Jacobs JJ. In vivo corrosion of modular hip prosthesis components in mixed and similar metal combinations. The effect of crevice, stress, motion, and alloy coupling. *J Biomed Mater Res* 1993;27(12):1533.
- [23] Brown SA, Flemming CA, Kawalec JS, et al. Fretting corrosion accelerates crevice corrosion of modular hip tapers. *J Appl Biomater* 1995;6(1):19.
- [24] Rodrigues DC, Urban RM, Jacobs JJ, Gilbert JL. In vivo severe corrosion and hydrogen embrittlement of retrieved modular body titanium-alloy hip implants. *J Biomed Mater Res B Appl Biomater* 2009;88:206.
- [25] Martin AJ, Jenkins DR, Van Citters DW. The role of corrosion in taper failure and head disassociation in total hip arthroplasty. *J Orthop Res* 2018;36:2996.
- [26] Martin AJ, McGrory BJ, Edidin AA, Van Citters DW. Using coordinate measuring machine validated with white light interferometry to identify contributors to material loss due to corrosion of total hip replacement modular junctions. In: Mihalko WM, Lemons JE, Greenwald AS, Kurtz SM, editors. *ASTM STP 160: Beyond the implant; retrieval analysis methods for implant surveillance*. W. Conshohocken, PA: ASTM International; 2018. p. 118.
- [27] Jacobs JJ, Urban RM, Gilbert JL, et al. Local and distant products from modularity. *Clin Orthop Relat Res* 1995;(319):94.
- [28] Urban R, Jacobs JJ, Gilbert JL, et al. Characterization of solid products of corrosion generated by modular-head femoral stems of different designs and materials. In: Parr J, Marlowe D, Mayor M, editors. *Modularity of orthopaedic implants*. West Conshohocken, PA: ASTM International; 1997. p. 33–44.
- [29] Eltit F, Assiri A, Garbuz D, et al. Adverse reactions to metal on polyethylene implants: highly destructive lesions related to elevated concentrations of cobalt and chromium in synovial fluid. *J Biomed Mater Res A* 2017;105A:1876.
- [30] Langton D, Sidaginamale RP, Lord J, Joyce T, Natu S, Nargol A. Abstract: metal debris release from taper junctions appears to have greater clinical impact than debris released from metal on metal bearing surfaces. *Bone Joint J* 2013;95-B(Supplement 1):28.
- [31] McGrory BJ, Payson AM, MacKenzie JA. Elevated intra-articular hip cobalt and chromium levels in mechanically assisted crevice corrosion in metal-on-polyethylene total hip arthroplasty. *J Arthroplasty* 2017;32:1654.
- [32] Wyles CC, Paradise CR, Masters TL, et al. Cobalt and chromium ion release in metal-on-polyethylene and ceramic-on-polyethylene THA: a simulator study with cellular and microbiological correlations. *J Arthroplasty* 2019. [Epub ahead of print].
- [33] Morozov PP, Sana M, McGrory BJ, Farraher SJ, Abrahams TG. Comparison of pre-revision magnetic resonance imaging and operative findings in mechanically assisted crevice corrosion in symptomatic metal-on-polyethylene total hip arthroplasties. *J Arthroplasty* 2017;32:2535.
- [34] Fillingham YA, Della Valle CJ, Bohl DD, et al. Serum metal levels for the diagnosis of adverse local tissue reaction secondary to corrosion in metal-on-polyethylene bearing total hip arthroplasty. *J Arthroplasty* 2017;32: S272.
- [35] Jacobs JJ, Cooper HJ, Urban RM, Wixson RL, Della Valle CJ. What we know about taper corrosion in total hip arthroplasty. *J Arthroplasty* 2014;29:668.
- [36] Kwon YM, Khormae S, Liow MHL, Tsai TY, Freiberg AA, Rubash HE. Asymptomatic pseudotumors in patients with taper corrosion of a dual-taper modular femoral stem. *J Bone Joint Surg Am* 2016;98:1735.
- [37] Kwon YM, MacAuliffe J, Arauz PG, Peng Y. Sensitivity and specificity of metal ion level in predicting adverse local tissue reactions due to head-neck taper corrosion in primary metal-on-polyethylene total hip arthroplasty. *J Arthroplasty* 2018;33:3025.
- [38] Lencioni A, Ellis B, Dean C, Lendrum J, Hogan C. Metal-on-metal total hip arthroplasty adverse local tissue reaction with intermittent unilateral vascular claudication. *Arthroplasty Today* 2019;5:389.
- [39] Zink T, McGrory BJ. Taper corrosion in a metal-on-polyethylene total hip presenting with lower extremity vascular compromise. *Arthroplasty Today* 2020. Submitted.
- [40] Jacobs J. Corrosion at the head-neck junction: why is this happening now? *J Arthroplasty* 2016;31:1378.